

WO9413268

Publication Title:

METHOD AND DEVICE FOR TREATING AND ENLARGING BODY LUMENS

Abstract:

Abstract of WO9413268

The present invention relates generally to stents (2) having delivery matrices which provide for the controlled release of bioactive substances. The delivery matrices comprise porous and erodible filaments (54), and multiple filaments may be employed in order to release different bioactive substances and/or the same bioactive substance at different delivery rates. The stents (2) are particularly useful for preventing restenosis of dilated body lumens, such as blood vessels. Methods for preventing stenosis of dilated body lumens or locally delivering bioactive compounds to tissue are also provided.

Data supplied from the esp@cenet database - Worldwide

Courtesy of <http://v3.espacenet.com>

This Patent PDF Generated by Patent Fetcher(TM), a service of Stroke of Color, Inc.




INTERNATIONAL APPLICATION PUBLISHED UNDER THE PATENT COOPERATION TREATY (PCT)

<p>(51) International Patent Classification⁵: A61K 9/22</p>	<p>A1</p>	<p>(11) International Publication Number: WO 94/13268</p> <p>(43) International Publication Date: 23 June 1994 (23.06.94)</p>
<p>(21) International Application Number: PCT/US93/11358</p> <p>(22) International Filing Date: 22 November 1993 (22.11.93)</p> <p>(30) Priority Data: 07/985,382 4 December 1992 (04.12.92) US</p> <p>(71)(72) Applicant and Inventor: KAPLAN, Aaron, V. [US/US]; 851 Carnation Court, Los Altos, CA 94024 (US).</p> <p>(74) Agent: HESLIN, James, M.; Townsend and Townsend Kourie and Crew, One Market Plaza, 20th floor, Stuart Street Tower, San Francisco, CA 94105 (US).</p>		<p>(81) Designated States: AU, CA, JP, KR, NZ, European patent (AT, BE, CH, DE, DK, ES, FR, GB, GR, IE, IT, LU, MC, NL, PT, SE).</p> <p>Published <i>With international search report. Before the expiration of the time limit for amending the claims and to be republished in the event of the receipt of amendments.</i></p>

(54) Title: METHOD AND DEVICE FOR TREATING AND ENLARGING BODY LUMENS

(57) Abstract

The present invention relates generally to stents (2) having delivery matrices which provide for the controlled release of bioactive substances. The delivery matrices comprise porous and erodible filaments (54), and multiple filaments may be employed in order to release different bioactive substances and/or the same bioactive substance at different delivery rates. The stents (2) are particularly useful for preventing restenosis of dilated body lumens, such as blood vessels. Methods for preventing stenosis of dilated body lumens or locally delivering bioactive compounds to tissue are also provided.

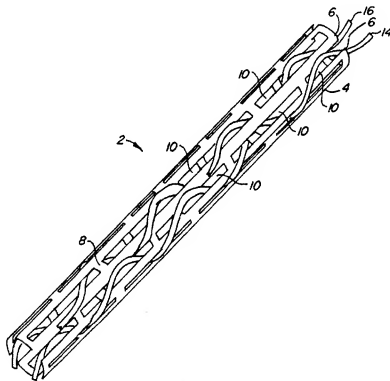

FOR THE PURPOSES OF INFORMATION ONLY

Codes used to identify States party to the PCT on the front pages of pamphlets publishing international applications under the PCT.

AT	Austria	GB	United Kingdom	MR	Mauritania
AU	Australia	GE	Georgia	MW	Malawi
BB	Barbados	GN	Guinea	NE	Niger
BE	Belgium	GR	Greece	NL	Netherlands
BF	Burkina Faso	HU	Hungary	NO	Norway
BG	Bulgaria	IE	Ireland	NZ	New Zealand
RJ	Benin	IT	Italy	PL	Poland
BR	Brazil	JP	Japan	PT	Portugal
BY	Belarus	KE	Kenya	RO	Romania
CA	Canada	KG	Kyrgyzstan	RU	Russian Federation
CF	Central African Republic	KP	Democratic People's Republic of Korea	SD	Sudan
CG	Congo	KR	Republic of Korea	SE	Sweden
CH	Switzerland	KZ	Kazakhstan	SI	Slovenia
CI	Côte d'Ivoire	LI	Liechtenstein	SK	Slovakia
CM	Cameroon	LK	Sri Lanka	SN	Senegal
CN	China	LU	Luxembourg	TD	Chad
CS	Czechoslovakia	LV	Latvia	TG	Togo
CZ	Czech Republic	MC	Monaco	TJ	Tajikistan
DE	Germany	MD	Republic of Moldova	TT	Trinidad and Tobago
DK	Denmark	MG	Madagascar	UA	Ukraine
ES	Spain	ML	Mali	US	United States of America
FI	Finland	MN	Mongolia	UZ	Uzbekistan
FR	France			VN	Viet Nam
GA	Gabon				

METHOD AND DEVICE FOR TREATING AND ENLARGING BODY LUMENS
BACKGROUND OF THE INVENTION

1. Field of the Invention

5 The present invention relates generally to intraluminal stents. More particularly, the present invention provides devices and methods which allow for localized delivery of bioactive compounds.

10 Many diseases may cause body lumens to undergo stenosis. Probably the most common is atherosclerosis. Atherosclerosis is a condition which commonly affects the coronary arteries of the heart, the aorta, and the carotid arteries. Atherosclerotic plaques of lipids, fibroblasts, and fibrin proliferate and cause obstruction of the artery. As
15 the obstruction increases, a critical level of stenosis is reached which does not allow sufficient blood flow to pass the obstruction to meet the metabolic needs of tissue distal to the obstruction resulting in ischemia. Atherosclerotic plaques also have the potential for rupture which can expose
20 the flowing blood to a strong procoagulant stimuli often resulting in thrombus formation. Thrombus formation in the coronary circulation leads to unstable angina and myocardial infarction. Thrombus formation in the cerebral circulation leads to stroke, TIA (transient ischemic attack) and RIND
25 (reversible ischemic neurologic deficit).

 Many therapeutic alternatives are available for the treatment of atherosclerotic diseases, including surgery and medical treatment. One particularly useful therapy for selected atherosclerotic lesions is percutaneous transluminal angioplasty. During angioplasty, a balloon tipped catheter is
30 inserted in an artery of the patient with the balloon deflated. The catheter tip is advanced to the site of the atherosclerotic plaque to be dilated. The balloon is placed within the stenotic segment of the artery and inflated.
35 During inflation the plaque "cracks" and the vessel expands, at least partially relieving the stenosis.

While angioplasty has gained wide acceptance, it suffers from two major problems, i.e. abrupt closure and restenosis. Abrupt closure refers to the acute occlusion of a vessel immediately after or within the initial hours following a dilatation procedure. Abrupt closure occurs in approximately one in twenty cases and frequently results in myocardial infarction and death if blood flow is not restored in a timely manner. The primary mechanisms of abrupt closures are arterial dissection and/or thrombosis. It is postulated, that the ability to deliver agent (e.g. antithrombotic) directly into the arterial wall at the time of angioplasty could reduce the incidence thrombotic acute closure.

Restenosis refers to the re-narrowing of an artery after an initially successful angioplasty. Restenosis occurs within the initial six months after angioplasty and is due to the proliferation and migration of the cellular components of the arterial wall. It is postulate that the delivery of agent(s) directly into the arterial wall would interrupt the cellular events leading to restenosis.

Medical prevention of abrupt closure and restenosis has not been entirely successful. Endovascular stents have been placed in the dilated segments to mechanically block abrupt closure and restenosis. Unfortunately, such stents have a high rate of thrombotic abrupt closure and have not significantly reduced restenosis.

Non-atherosclerotic vascular stenosis may also be treated by angioplasty. For example, Takayasu arteritis or neurofibromatosis may cause stenosis by fibrotic thickening of the arterial wall. Restenosis of these lesions occurs at a high rate following angioplasty, however, due to the fibrotic nature of the diseases. Medical therapy has been similarly disappointing.

What is needed in the art are devices and methods for the prevention of abrupt closure and/or restenosis following dilation of blood vessels. In particular, it would be desirable to provide devices and methods which can provide antithrombotic and other medications to regions of a blood

vessel which have been treated by angioplasty or other interventional techniques, such as atherectomy, laser ablation, or the like. Such devices should be capable of providing both short term medication delivery, over the
5 initial hours and days after the treatment, as well as long term medication delivery, over the weeks and months after the treatment. Surprisingly, the present invention fulfills these and other needs.

2. Description of the Background Art

10 U.S. Patent No. 4,300,244 describes an endovascular prosthesis which may be coated with carbon for biocompatibility. U.S. Patent No. 4,580,568 describes endovascular stents which are formed of stainless steel in a zig-zag pattern. U.S. Patent No. 4,733,665 describes
15 expandable intraluminal vascular grafts placed by balloon angioplasty catheters. U.S. Patent No. 4,739,762 describes expandable intraluminal grafts which may have a plurality of slots in the graft walls. U.S. Patent No. 4,776,337 describes expandable intraluminal stents coated with a biologically
20 inert substance, such as polyurethane or other inert plastics. U.S. Patent No. 4,800,882 describes an expandable endovascular stent formed from wire bent into serpentine configurations. U.S. Patent No. 4,990,155 describes a plastic coil for use as an endovascular stent to prevent restenosis following
25 angioplasty. U.S. Patent No. 5,019,090 describes radially expandable endoprostheses. U.S. Patent No. 5,053,048 describes thromboresistant coating which may be applied to intravascular stents. U.S. Patent No. 5,059,211 describes expandable endovascular stents which are bioabsorbable. Each
30 of the above references is incorporated herein by reference.

PCT Application No. 92/11895 describes a balloon catheter capable of releasing drugs directly to tissue in a body lumen wall. PCT Application No. WO 92/11890 describes a
35 balloon catheter having a coating of body affecting chemicals which are released when the balloon is inflated and contacted with body lumen walls. PCT Application No. WO 87/04935 describes spring coil intravascular stents. European Patent

Publication No. 281,482 describes preparation of biodegradable polymers. European Patent Publication No. 433,011 describes an intra-arterial stent which incorporates or is coated with a radioisotope. Chasin et al., "Polyanhydrides as Drug Delivery Systems" in *Biodegradable Polymers as Drug Delivery Systems*, Langer and Chasin, eds., Marcel Dekker, Inc., 1990, pp. 43-70; Langer, Science, 249:1527-1532; and Langer and Moses, J. Cell. Biochem., 45:340-345 describe biodegradable materials useful in drug delivery systems. Each of the above references is incorporated herein by reference.

SUMMARY OF THE INVENTION

The present invention provides endovascular stents and methods for delivering therapeutic and other substances to selected locations within a patient's vascular system. The endovascular stent comprises a tubular structure having an initial diameter and being expandable from the initial diameter to an enlarged diameter. A delivery matrix including at least one filament is interlaced with the tubular structure and expandable therewith from the initial diameter to the enlarged diameter. A bioactive substance is releasably contained within the filament of the delivery matrix, and is released from said matrix when exposed to the conditions present in the vascular system.

The tubular structure may be composed of an elastic material, such as an elastomer polymer, whereby the tubular structure may be initially constrained to set initial diameter and thereafter released to said enlarged diameter. Alternatively, the tubular structure could be composed of a non-plastic material, whereby the tubular structure may be expanded from the initial diameter to the enlarged diameter, typically using a balloon dilatation catheter. The various specific designs for the tubular structure exit, including a helical structure where the filament of the delivery matrix is counter woven with a helical strand of the tubular structure, a helical structure where the filament is laminated to a helically wound strand of the tubular structure, and a perforated cylinder where the filament of the delivery matrix

is interwoven through perforations in the cylinder. The filament of the delivery matrix may be porous and substantially non-erodible, where the bioactive substance is absorbed or impregnated therein and released over time.

Alternatively, the filament will be composed of the material which is erodible within the vascular environment, where the bioactive substance is contained or dispersed in the filament and released as the filament material erodes.

In a preferred embodiment of the endovascular stent, the delivery matrix will include at least one first filament and at least one second filament, where the first and second filaments are both interlaced with the tubular structure and expandable therewith. Usually, the first and second filaments will have differing characteristics so that the first filament will release a bioactive substance contained therein over a first time period and the second filament will release a bioactive substance contained therein over a second time period. In this way, a single bioactive substance can be delivered over two independent profiles, and/or two different bioactive substances may be delivered simultaneously or over different delivery profiles.

According to the method of the present invention, a stent is inserted into a body lumen to delivery a bioactive substance. The stent is constructed as described above and is expanded at a location within the body lumen selected to be treated. After such placement, the bioactive substance(s) are released according to the mechanisms described above.

BRIEF DESCRIPTION OF THE FIGURES

Fig. 1A illustrates a perspective view of a stent prior to expansion having two stands woven through the perforations.

Fig. 1B illustrates a view through the interior of a stent prior to expansion having two strands woven through the perforations.

Fig. 1C illustrates a close-up perspective view of a stent having two strands woven through the perforations prior to expansion.

Fig. 2A illustrates a perspective view of a stent following expansion having two stands woven through the perforations.

5 Fig. 2B illustrates a view through the interior of a stent following expansion having two strands woven through the perforations.

Fig. 2C illustrates a close-up perspective view of a stent having two strands woven through the perforations following expansion.

10 Fig. 3A illustrates a perspective view of a stent following expansion having two pairs of stands woven through the perforations.

Fig. 3B illustrates a view through the interior of a stent following expansion having two pairs of strands woven through the perforations.

15 Fig. 3C illustrates a close-up perspective view of a stent having two pairs of strands woven through the perforations following expansion.

20 Fig. 4A illustrates a perspective view of a stent structure comprising a single helically wound strand and two counterwound delivery matrix filaments.

Fig. 4B is a cross-sectional view taken along line 4B-4B of Fig. 4A.

25 Fig. 5A is a side elevational view of a stent comprising a single helically wound strand having a pair of delivery matrix filaments laminated thereto.

Fig. 5B is a detailed cross-sectional view illustrating a first configuration for laminating the filaments onto the strand of Fig. 5A.

30 Fig. 5C is a detailed cross-sectional view illustrating a second configuration for laminating the filaments onto the strand of Fig. 5A.

35 Fig. 6A-6C illustrate the method of the present invention for positioning the endovascular stent of Figs. 4A and 4B in a blood vessel in order to deliver a bioactive substance therein. The stent is delivered with a balloon

dilatation catheter and a stenosed region is dilated as a result of the procedure.

DETAILED DESCRIPTION OF THE SPECIFIC EMBODIMENTS

5 The present invention provides devices and methods for treating body lumens particularly for preventing restenosis of blood vessels following dilation of stenotic segments. The devices and methods also provide a means for delivering bioactive substances and compounds in a localized manner.

10 According to the present invention, an endovascular stent comprises a tubular structure having an initial diameter and being expandable from the initial diameter to an enlarged diameter. For most vascular applications, the initial diameter will be in the range from about 1.25 mm to 2 mm,
15 usually being from about 1.25 mm to 1.5 mm. The final enlarged diameter will usually be in the range from about 2 mm to 6 mm, more usually being from 2 mm to 4 mm. The tubular structure can have any of a variety of conventional stent structures, such as helically wound strands, perforated
20 cylinders or the like. The number of specific structures are disclosed in the background patents which are listed above and which have been incorporated herein by reference.

Endovascular stent will further comprise a delivery matrix for containing and releasing a bioactive substance into
25 the body lumen being treated, typically a blood vessel. The delivery matrix will include at least one filament which is interlaced with the tubular structure which is expandable therewith from the initial diameter to the enlarged diameter. It will be appreciated that the tubular structure acts as a
30 mechanical support for the delivery matrix, thus allowing a wide variety of materials to be utilized as the delivery matrix.

By "bioactive substance", it is meant that the compound exerts a biological effect on the tissue of the host.
35 The biological effect will generally be local in nature, i.e. only occurring very close to the strand, but may also exert biological effects more distantly. The biological effects may

include anti-proliferative activity, thrombotic inhibition, inhibition of vasospasm, or the like.

The tubular structure may be composed of a variety of bio-compatible materials. Typically, the tubular member
5 may be stainless steel; silver; tantalum; gold; titanium; tungsten; platinum; polymers, such as polyether sulfone, polyamide, polycarbonate, polypropylene, high molecular weight polyethylene; carbon fiber; and the like. When the tubular
10 member is constructed of radiolucent materials, such as polypropylene or polyethylene, a radiopaque coating may be applied to the stent. The radiopaque coating provides a means for identifying the location of the stent by plain x-rays or fluorography during or after stent placement.

The tubular structure will generally have non-
15 elastic (plastic) properties in that it will retain its shape following expansion. This provides a means for controlled expansion in the body lumen. In these embodiments, an outward force applied from the interior of the stent will increase the diameter of the tubular member. The degree of radial
20 expansion can be controlled by the amount of force exerted. Angioplasty balloon catheters provide a means for controlling the force, and hence the expansion, of the tubular member. The catheter balloon can be expanded to predetermined pressures in order to expand the tubular member.

25 Alternatively, the tubular structure can have elastic properties. In these embodiments, the tubular member is held in a contracted position for placement. Outward tension is created in the tubular member by the force contraction. When the stent is placed, the tension within the
30 tubular member causes expansion of the tubular member. The tubular member expands to securely contact the lumen wall.

The tubular structure may be coated with a biologically inert coating. Examples of suitable inert coatings include porous polyurethane, Teflon®, or other
35 conventional biologically inert plastic substances. The coating should be thin and highly elastic so as not to interfere with expansion of the stent. The coating may also

have anchoring means for securing the stent to the inner wall of the body lumen. The anchoring means may be projections which extend radially outward from the outer surface of the tubular member.

5 In a first exemplary embodiment, the tubular structure will be a perforated cylinder. The perforations in the cylinder may be circular, ovoid, slots, or the like. The tubular structure may also be comprised of a helically wound or serpentine type wire structure. The turns or curves in the
10 wire are analogous to the perforations in the perforated cylinder, as described below.

 The perforations or open wire structure will permit expansion of the tubular structure. The solid portions of the perforated cylinder may be deformed by outward expanding
15 forces from within the tubular member. While the perforations allow deformation of the solid portions of the tubular member, the tubular member will retain the expanded shape following deformation under the naturally occurring forces within the body lumen.

20 The perforations may be formed in cylindrical members by etching or cutting through the solid walls. Conventional etching processes such as electromechanical or laser etching may be used. Alternatively, the tubular members may be constructed from a plurality of longitudinal members
25 joined to form a tubular structure. The longitudinal members may be joined by welding, soldering, brazing, or epoxy resins, depending on the composition of the longitudinal members. The longitudinal members will generally have a circular cross-sectional shape, but may also have a cross-sectional shape
30 which is triangular, square, rectangular, and the like. Horizontal members may also be employed to join the longitudinal members by similar means. By joining the longitudinal members at discrete points along their length, perforations are formed in the tubular member.

35 The perforations also provide a means for immobilizing the filaments of the delivery matrix in the tubular structure. The filaments contain bioactive compounds

which are released in a controlled fashion following placement of the stent. By interlacing the filament through the perforations of the tubular structure, the filaments are held in close contact with the wall of the body lumen by the expanded tubular member.


5 Generally, the filaments are polymers which are degradable over time, within the vascular environment. By "biodegradable polymer," it is meant that the polymer will naturally erode in a physiological environment. The bioactive compounds are mixed in the polymer and released as the polymer
10 degrades. Polymers may be synthesized with specific degradation characteristics determining the life span of the polymer under physiological conditions. The rate of polymer degradation and the concentration of bioactive compound in the
15 polymer determines the release rate of the bioactive compound to the surrounding tissue.

Methods of constructing polymers having desired degradation characteristics are generally known. For example, co-polymers of poly[bis(p-carboxyphenoxy) propane anhydride]
20 and sebacic acid may be synthesized to yield desired biodegradation characteristics. Pure poly[bis(p-carboxyphenoxy) propane anhydride] has a relatively low erosion rate. Co-polymerizing sebacic acid with poly[bis(p-carboxyphenoxy) propane anhydride] increases the erosion rate.
25 As sebacic acid content increases, the erosion rate may increase by a factor of several hundred. See Leong et al., J. Biomed. Mat. Res., 19:941-955 (1985), incorporated herein by reference. Thus by altering the relative content of each of the components, co-polymers having the desired degradation
30 characteristics may be synthesized.


Many biocompatible polymers are known, including several which are biodegradable. Several are described in Langer, Science, 249:1527-1532 (1990) and Langer and Moses, J. Cell. Biochem., 45:340-345 (1991), both of which are
35 incorporated herein by reference. Poly-L-lactide polymers degrade over a period of months under physiological conditions. Lactic acid-glycolic acid co-polymers are also

well known biodegradable polymers. Other acceptable polymers may contain monomers of hydroxyethylmethacrylate, vinylalcohol, ethylene-vinylacetate, lactic acid, or glycolic acid.

- 5 Particularly useful polymers in the present invention are polyanhydrides of the general formula



where x varies from 1 to 10 or



- 10 as generally described in Chasin et al., "Polyanhydrides as Drug Delivery Systems" in *Biodegradable Polymers as Drug Delivery Systems*, Langer and Chasin, eds. Marcel Dekker, Inc. 1990, pp. 43-70, incorporated herein by reference. Polymers comprising monomers such as carboxyphenoxyacetic acid,
15 carboxyphenoxyvaleric acid, carboxyphenoxyoctanoic acid, terephthalic acid, and carbophenoxy propane-sebacic acid are examples of polymers acceptable for use in the present invention.

- Polymers containing bioactive compounds may be
20 formulated by a variety of methods well known in the art. For example, polymer matrices having the bioactive compounds incorporated within the matrices may be formulated by molding procedures. Briefly, polymer is ground and sieved to a desired particle size, usually about 90-150 μm . The bioactive
25 compounds are ground and sieved to the same particle size and mixed with the polymer particles. The mixture is injection molded in commercially available molders. The polymer containing bioactive compounds is thus formed into strands and ready for weaving into the tubular member.

- 30 The strands may have a variety of cross-sectional shapes and dimensions which may be varied to control the release of the bioactive compound. Typically, the strands will have a circular cross-section although other cross-sectional shapes such as rectangular or ovoid are also
35 acceptable.

 The strands are woven through the perforations of the tubular member. At least one strand is woven through the

perforations of each tubular member. Often multiple strands of different materials are woven through the perforations of each tubular member. Different strands may also contain different bioactive compounds. By placing different bioactive compounds in strands of different materials, stents of the present invention may be constructed which will release the different bioactive compounds at different rates, each in a controlled manner.

As an alternative to biodegradable polymers, the present invention can employ filaments of non-degradable materials which permit controlled release of the bioactive substances therefrom within the vascular environment. Suitable non-erodible polymers include styrene-divinyl benzene copolymer, methyl methacrylate-ethylene glycol and dimethylmethacrylate copolymer and ethylene-vinyl acetate copolymer. Filaments may be formed by extrusion of such copolymeric resins, typically having dimensions in the range from about 0.04 mm to 0.4 mm.

The delivery matrix of the present invention is suitable for the delivery of a variety of pharmaceutical and other therapeutic agents including organic molecules, proteins, peptides, nucleotides, carbohydrates, polysaccharides, mucopolysaccharides, simple sugars, glycosaminoglycans, steroids and the like. The agents delivered may perform a variety of functions, including antithrombotic (e.g., lytic agents such as recombinant tissue plasminogen activator (TPA), urokinase and streptokinase), antiplatelet agents (aspirin, ticlopidine), inhibitors or surface glycoprotein receptors (e.g., GP IIb/IIIa, GP Ib-IX), antimetabolites (e.g. methotrexate), growth factor inhibitors, growth factor promoters, anticoagulants (e.g., heparin, low molecular weight heparins), direct thrombin inhibitors (e.g. hirudin and its derivatives, hirulog, thrombin aptamer, argatroban, D-phenylalanyl-L-poly-L-arginyl chloromethyl ketone), antimitotics (e.g., colchicine), antibiotics, antisense nucleotides, and the like.

Some embodiments of the present invention will comprise strands containing different bioactive substances or compounds. The strands containing the different bioactive compounds may be comprised of the same or different materials. When the strands are comprised of biodegradable polymers, use of a different polymeric formulation or a different polymer system provides a method of releasing the bioactive compounds at different rates. Alternatively, the same polymer may be used to provide for similar rates of release of different bioactive compounds.

Stents of the present invention may be useful in a variety of clinical settings. A common use of the present invention is for prevention of restenosis of coronary arteries following dilation of a stenotic arterial segment by transluminal procedures such as angioplasty. The intracoronary stents will generally have two types of biodegradable strands. An anticoagulant, usually heparin, will be contained within one strand. The heparin prevents thrombus formation caused by injury to the vessel during angioplasty or from foreign body reaction caused by the stent. The heparin containing strand degrades relatively quickly, usually within two to three weeks. This provides time for natural re-endothelialization to occur which will isolate the stent and injured vessel components from blood in the vascular space, and hence remove the thrombotic stimulus. The second strand will usually contain an antiproliferative agent such as methotrexate. The antiproliferative agent will inhibit overproliferation of smooth muscle cells and thus inhibit restenosis of the dilated segment of the vessel. The antiproliferative containing strand will generally degrade over a period of four to six months. The physical presence of the stent will also inhibit re-stenosis of the vessel. In some applications the stents may have a third strand which contains a vasodilator such as a calcium channel blocker or a nitrate. The vasodilator will suppress vasospasm which is common following angioplasty procedures. The vasospasm occurs as a response to injury of the vessel. As the vessel heals,

the tendency toward vasospasm decreases. The vasodilator strand will generally degrade in about two to three weeks. Stents may be placed in other blood vessels, such as the aorta, carotid arteries, renal, iliac, or peripheral arteries for similar purposes.

Stents of the present invention have other uses also. Stents of the present invention may be employed to provide controlled release of compounds to localized areas. For example, arterio-venous malformations may be treated by placement of a stent of the present invention. The stent will generally have one strand type which contains an irritant that naturally induces inflammation and fibrosis. On such irritant is tetracycline which can irritate the blood vessel leading to the malformation causing thrombosis and fibrotic closure of the malformation.

Stents of the present invention may also be used to deliver relatively high doses of anti-cancer chemotherapeutic agents to a localized tumor. For example, stents may contain several different strands containing different chemotherapeutic agents. The stents may be placed in the artery supplying blood to the tumor. The tumor can then be treated with relatively high and prolonged doses of the chemotherapeutic agents while limiting systemic toxicity. The stent may be used as a curative treatment, for pre-operative debulking, or for palliation of symptoms.

In another embodiment neurological disorders such as Parkinson's disease may be treated with stents of the present invention. In Parkinson's disease, dopamine or dopamine agonists, such as bromocriptine mesylate or pergolide mesylate, may be the bioactive compounds contained in biodegradable strands. The stents may be placed in the vascular supply of the thalamic substantia nigra. As the strands erode, the bioactive compound is released and flows into the substantia nigra providing localized treatment of the thalamus.

The stents of the present invention may also find use in body lumens other than blood vessels. One example is

to preserve the integrity of the common bile duct in patients having primary cholangiosarcoma, secondary invasion of the duct by other tumors, or stone disease. Stents having strands containing antiproliferative agents may be placed in the common bile duct to prevent stenosis or restenosis resulting from malignancies such as pancreatic cancer. The stent may also find use in the treatment of genito-uretal disorders involving organs such as the prostate (benign prostatic hypertrophy or carcinoma via the prostatic urethra), penis (strictures via the penile urethra), fallopian tubes and the like. Persons of skill will appreciate that the stents of the present invention may be used in a wide variety of other clinical situations.

Stents of the present invention will generally not require open surgical placement. For example, stents to prevent restenosis of coronary arteries will generally be placed by transluminal angioplasty catheters. Generally, following angioplasty the stent will be directed to the dilated site by a balloon catheter. The stent, will be securely placed over the balloon. When the stent is within the dilated segment, the balloon will be inflated and the stent will expand to securely contact the vessel wall. As the balloon deflates, the stent retains its expanded form and remains securely in contact with the vessel wall. The deflated balloon can be withdrawn from the interior of the stent, leaving the stent in place. Placement of stents of the present invention in other locations may be similarly achieved. Alternatively, stents may be placed during open surgical procedures and perform similar functions.

Methods for preventing stenosis or restenosis of bodily fluid lumens are also provided. Hereinafter, the phrase "bodily fluid lumens" refers to body cavities which contain or transmit body fluids. This includes, but is not limited to, both arterial and venous blood vessels, the common and cystic bile ducts, the ureters, the urethra, central nervous system ventricles, and the like. Segments of bodily fluid lumens which have been dilated or which are at risk for

stenosis may be protected from occlusion by inserting a stent comprising a tubular member having a radius, a first end, a second end, and a wall surface defining an interior of the tubular member, wherein the wall surface contains a plurality of perforations which allow the radius of the tubular member to be expanded by an outwardly expanding force from the interior, and an anti-proliferative compound contained in at least one first strand woven through perforations in the wall surface, into the dilated luminal segment; and expanding the stent to circumferentially contact the wall of the dilated segment of the lumen.

The method of lumen dilation is not critical and may vary. Generally stents of the present invention will be placed in dilated lumen segments by closed procedures, such as by placement by percutaneous transluminal angioplasty catheters in coronary arteries or by endoscopic placement in the common bile duct. Alternatively, the stents may be placed in lumen segments which have been surgically enlarged, e.g., placement in arteries following endarterectomy procedures.

The stent is positioned in the lumen so that the first end and the second end of the tubular member extend past the dilated lumen segment. In some embodiments of the present invention, an outward force is applied to the interior wall surface of the tubular member causing the tubular member to radially expand. The tubular member contacts the interior wall of the lumen. The pressure applied to the interior wall of the lumen by the tubular member may be controlled by controlling the amount of force applied to the interior of the tubular member. Conveniently, the force is applied by a inflation of a balloon catheter, such as an angioplasty catheter, within the tubular member. Following expansion of the tubular member, the balloon is deflated and withdrawn. The stent is held in place by the pressure of the tubular member on the interior wall of the lumen. While stents of the present invention will generally be placed following dilation of a stenotic segment, the stent may be placed in the stenotic

segment and expanded simultaneous to dilating the stenotic segment.

In an alternative embodiment, the stent will be self-expanding and have elastic properties. The tubular member will be contracted and placed within the distal end of a catheter having a means to expel the stent from the distal end. Contraction of the stent causes outward tension in the tubular member, so that upon expulsion from the catheter the tubular member will radially expand and contact the lumen wall. Following expulsion of the stent, the catheter may be withdrawn. The outward tension of the tubular member will hold the stent in position in the lumen.

The present invention also provides methods for localized delivery of a bioactive compound to the interior of a body lumen. Localized delivery of bioactive compounds is useful in many clinical settings which determine the choice of bioactive compound contained in the stent. Localized delivery of antiproliferative agents is particularly useful for the treatment of a variety of malignant conditions characterized by highly vascular growth. In these instances, stents of the present invention may be placed in the arterial supply of the tumor to provide a means of relatively high dose delivery of the antiproliferative agent to the tumor. Generally the methods comprise inserting a stent comprising a tubular member having a radius, a first end, a second end, and a wall surface defining an interior of the tubular member, wherein the wall surface contains a plurality of perforations which allow the radius of the tubular member to be expanded by an outwardly expanding force from the interior, and at least one strand which contains the bioactive compound is woven through perforations in the wall surface; and expanding the stent to circumferentially contact the wall of the lumen. Placement of the stent is similar to the methods described above.

Reference will now be made to the figures. Uniform reference numbers will be used for corresponding elements in different figures. It will be understood that no limitation

of the scope of the invention is intended and the figures are for illustrative purposes only. Alterations and modifications of the stents illustrated in the figures are contemplated to be within the scope of the invention.

5 In Figs. 1A-1C, a stent 2 constructed in accordance with the principles of the present invention is shown. Fig. 1A illustrates a perspective view of the entire length of the stent 2 prior to expansion. The stent 2 is comprised of a tubular member 4. In this embodiment, the tubular member 4 is
10 constructed from longitudinal elements 6 joined to form a tubular configuration by horizontal elements 8. Perforations 10 are formed by the spaces between the longitudinal elements 6 and horizontal elements 8. The tubular member 4 defines an interior 12 of the stent 2 which has a diameter d (see Fig. 1B).
15 1B).

As exemplified in Fig. 1C, the stent 2 contains two strands 14 and 16. The strands 14 and 16 are woven into the perforations 10 of the stent 2. The strands 14 and 16 are composed of different biodegradable polymers and contain
20 different bioactive substances.

Figs. 2A-2C illustrate the stent 2 of Fig. 1 following expansion. In Fig. 2A the longitudinal elements 6 have been deformed by the expansion. The longitudinal elements 6 remain joined by the horizontal elements 8. The
25 perforations 10 have been widened by the expansion. The interior 12 of the stent 2 has an increased diameter d' which will provide for secure contact to be made between the tubular member 4 and the body lumen wall (See Fig. 2B).

As illustrated in Fig. 2C, the strands 14 and 16
30 remain woven through the perforations 10. Also, the strands 14 and 16 remain in close contact to the tubular member 4 so as to avoid obstruction of the interior 12 of the tubular member and to remain close to the body lumen wall.

Figs. 3A-3C illustrate one stent 2 of the present
35 invention having four strands 14, 16, 18, and 20. The stent 2 is illustrated in an expanded configuration for clarity. Each of the strands 14, 16, 18, and 20 is woven through different

perforations 10 in the tubular member 4. The four strands 14, 16, 18, and 20 provide for delivery of a greater amount of bioactive compound to a larger surface area of the lumen wall than stents having two strands of similar composition.

5 Otherwise, the stent 2 functions similarly to stents with two strands.

Referring now to Figs. 4A and 4B, an alternative stent structure 50 comprising a helically wound strand 52 and a pair of counter-wound filaments 54 and 56 is illustrated.

10 The strand 52 may be composed of either an elastic or a non-elastic material. Typically, strand 52 will be composed of a non-elastic, such as a biocompatible metal, which may be placed within the vascular system using balloon dilation catheter as described hereinafter in connection with Fig. 6A-

15 6C. A strand 52 will typically be a wire having a circular cross-section, with a diameter of the range from about 0.05 to 0.25 mm.

The counter-wound delivery matrix filaments 54 and 56 may be composed of any of the materials described above, typically extruded or otherwise formed into elongate filaments

20 which are counter wound and secured to the tubular strand 52 at crossing points. Securing may be achieved by adhesives, the application of heat, or the like.

Referring now to Figs. 5A-5C, the second alternative structure 60 of the endovascular stent of the present invention will be described. The stent 60 also comprises a helical strand 62 which forms the tubular structure of the stent. The helical strand may be composed of an elastic or non-elastic material, as described generally above. Instead

25 of counter-wound filaments, as described above for stent 50, stent 60 includes a laminated filaments 64, as best observed in Figs. 5B and 5C. The filaments are composed of any of the materials described above for the delivery matrix filaments, which filaments are then laminated to the sides of the helical

30 strand 62 by conventional techniques, such as adhesives, heat lamination, or the like. In the case of Fig. 5B, the strand 62 has a circular cross-section, and a pair of filaments 64

35

are shaped to conform to the concave surface presented by the strand. In the case of Fig. 5C, the strand 62' has a pair of flat opposed faces, and the filaments 64' are formed to secure to such flat faces.

5 Referring now to Figs. 6A-6C, a balloon dilatation catheter 70 may be used to deliver the stent 50 to region of Stenosis and a Blood Vessel. The stent 50 is initially carried in its initial (or reduced) diameter configuration on an uninflated balloon 72 of the balloon catheter 70. The
10 balloon catheter is introduced over a conventional guidewire 74 and the stent 50 is positioned within the region of Stenosis using fluoroscopic imaging.

After the stent 50 is properly positioned within the region of Stenosis as illustrated in Fig. 6A, the balloon 72
15 will be inflated to expand the stent 50 within the region of Stenosis as illustrated in Fig. 6B. Stent 50 is composed of a non-elastic material, and will assume the enlarged configuration, as illustrated. The balloon 72 may then be deflated, and the catheter 70 may be withdrawn over the
20 guidewire 74. After removal of the guidewire 74, the expanded stent 50 will be left in place, as illustrated in Fig. 6C. The stent 50 will provide for mechanical support of the dilated stenosed region, in a manner conventional for vascular
25 stents. In addition, the stent 50 will provide one or more bioactive substances to the region immediately surrounding the region of dilation by releasing said substances from the filaments 54 and 56 (Figs. 4A and 4B) of the delivery matrix of the stent. The materials of the delivery matrix can be
30 selected to provide a desired bioactive substance delivery profile, with one or more bioactive substances being delivered at desired rates for desired time periods.

Although the foregoing invention has been described in detail for purposes of clarity of understanding, it will be obvious that certain modifications may be practiced within the
35 scope of the appended claims.

WHAT IS CLAIMED IS:

1. An endovascular stent comprising:
 - a tubular structure having an initial diameter, said
5 structure being expandable from the initial diameter to an enlarged diameter;
 - a delivery matrix including at least one filament which is interlaced with the tubular structure and expandable therewith from said initial diameter to said enlarged
10 diameter; and
 - a bioactive substance releasably contained within the filament of the delivery matrix.
2. An endovascular stent as in claim 1, wherein
15 said tubular structure is composed of an elastic material, whereby the tubular structure may be constrained to said initial diameter and thereafter released to said enlarged diameter.
3. An endovascular stent as in claim 1, wherein
20 said tubular structure is composed of a non-elastic material, whereby the tubular structure may be expanded from said initial diameter to said enlarged diameter.
4. An endovascular stent as in claim 1, wherein
25 the tubular structure includes at least one helically wound strand, and wherein the filament of the delivery matrix is counter-woven with said helically wound strand.
5. An endovascular stent as in claim 1, wherein
30 the tubular structure includes at least one helically wound strand, and wherein the filament of the delivery matrix is laminated over at least a portion of said helically wound strand.
6. An endovascular stent as in claim 1, wherein
35 the tubular structure includes a perforated cylinder, and

wherein the filament is interwoven through the perforations in said cylinder.

7. An endovascular stent as in claim 1, wherein
5 the filament is composed of a material which is biodegradable within a physiologic environment whereby the bioactive substance is released as the filament erodes within a blood vessel.

10 8. An endovascular stent as in claim 7, wherein the material is composed of at least one polymer system selected from the group consisting of lactic acid/glycolic copolymer, cobophenoxy propane/sebacic acid, polycaprolactones, polyanhydride and poly ortho-esters.

15 9. An endovascular stent as in claim 1, wherein the filament is composed of a material which is substantially biodegradable within a physiologic environment and elutes bioactive substances.

20 10. An endovascular stent as in claim 9, wherein the material is composed of at least one polymer selected from the group consisting of silicone, ethylene-vinyl acetate copolymer, poly (vinylalcohol).

25 11. A stent as in claim 1, wherein the bioactive substance is selected from the group consisting of organic molecules, proteins, peptides, nucleotides, carbohydrates, polysacchrides, mucopolysaccharides, simple sugar, glycoaminoglycans and steroids.

30 12. An endovascular stent comprising:
a tubular structure having an initial diameter, said structure being expandable from an initial diameter to an enlarged;
35

a delivery matrix including at least one first filament and at least one second filament, which first and

second filaments are interlaced with the tubular structure and expandable therewith from said initial diameter to said enlarged diameter; and

5 at least one bioactive substance releasably contained within both the first and second filaments.

13. An endovascular stent as in claim 12, wherein the first filament is composed of a first material selected to release the bioactive substance over a first time period and
10 wherein the second filament is composed of a second material selected to release the bioactive substance over a second time period.

14. An endovascular stent as in claim 13, wherein
15 at least one of the first and second filaments is composed of a porous material which is biodegradable within a vascular environment and elutes substances.

15. An endovascular stent as in claim 14, wherein
20 the material is composed of at least one polymer selected from the group consisting of lactic acid/glycolic copolymer, cobophenoxy propane/sebacic acid, polycaprolactones, polyanhydride and poly ortho-esters.

25 16. An endovascular stent as in claim 15, wherein both the first and second filaments are composed of the selected material.

30 17. An endovascular stent as in claim 13, wherein at least one of the first and second filaments is composed of a material which is substantially biodegradable within a vascular environment which elutes substances.

35 18. An endovascular stent as in claim 17, wherein the material is composed of at least one polymer selected from the group consisting of silicone, ethylene-vinyl acetate copolymer, poly (vinylalcohol).

19. An endovascular stent as in claim 18, wherein the first and second filaments are composed of the selected material.

5 20. A method for treating body lumens said method comprising:

 inserting into the body lumen a stent comprising (i) a tubular structure having an initial diameter, (ii) a delivery matrix including at least one filament interlaced
10 with the tubular structure, and (iii) a bioactive substance releasably contained within said filament; and

 expanding the stent at a location within the body lumen selected to be treated, whereby the bioactive substance
15 will be released from the filament under the conditions present in the immediate environment.

 21. A method as in claim 20, wherein the body lumen is a blood vessel and the selected location is a region of
20 stenosis.

 22. A method as in claim 21, wherein the bioactive substance is selected from the group consisting of organic
 molecules, proteins, peptides, nucleotides, carbohydrates, polysacchrides, mucopolysaccharides, simple sugar,
25 glycoaminoglycans, and steroids.

1/6

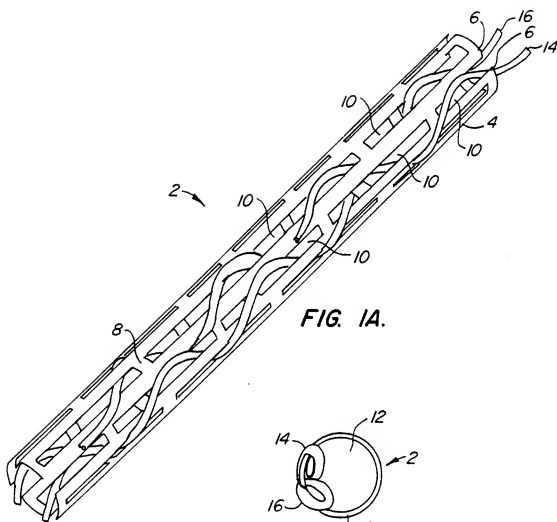


FIG. 1A.





FIG. 1B.



SUBSTITUTE SHEET (RULE 26)

FIG. 1C.

2/6




FIG. 2B.

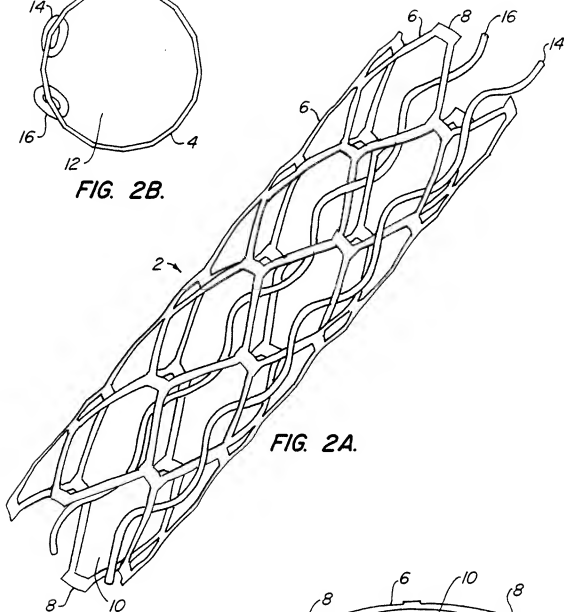


FIG. 2A.




FIG. 2C.

3/6




FIG. 3B.

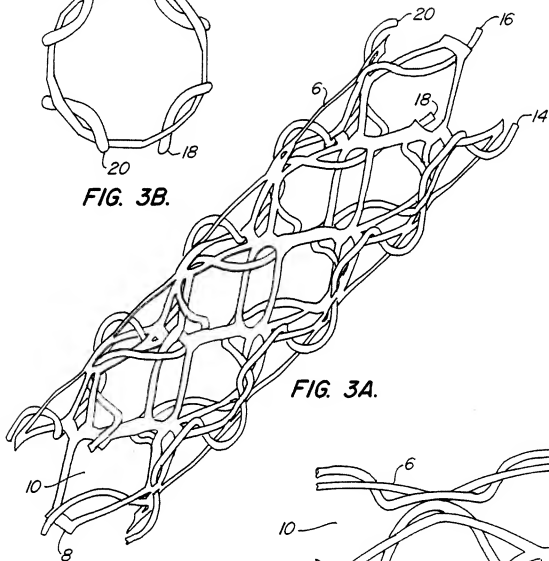


FIG. 3A.




FIG. 3C.

4/6

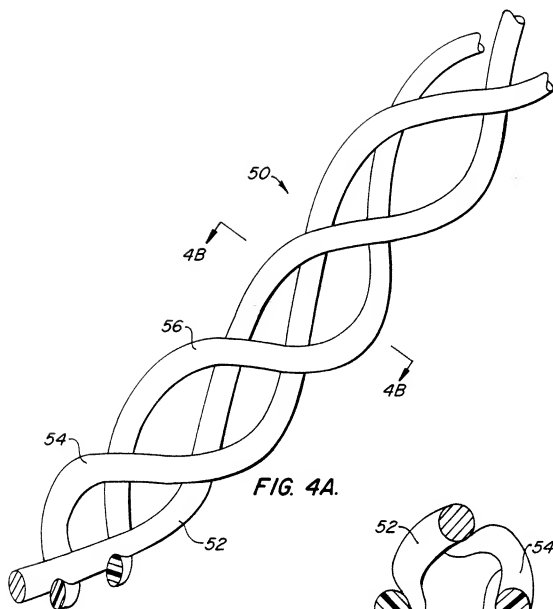


FIG. 4A.


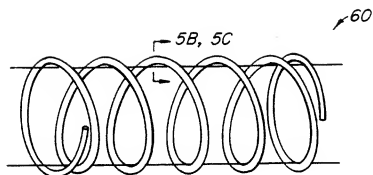




FIG. 4B.

5/6

**FIG. 5A.****FIG. 5B.****FIG. 5C.**

6/6

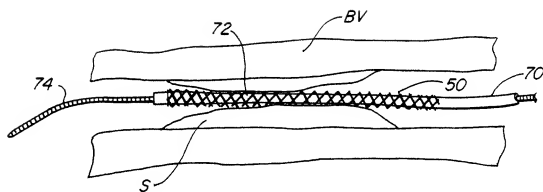


FIG. 6A.

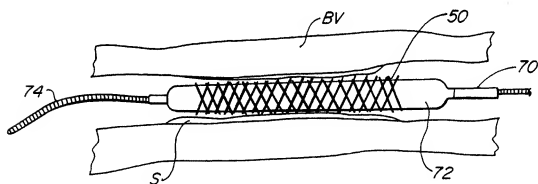


FIG. 6B.

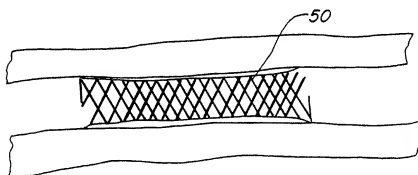


FIG. 6C.

INTERNATIONAL SEARCH REPORT

International application No.
PCT/US93/11358

A. CLASSIFICATION OF SUBJECT MATTER

IPC(5) : A61K 9/22

US CL : 604/891.1

According to International Patent Classification (IPC) or to both national classification and IPC

B. FIELDS SEARCHED

Minimum documentation searched (classification system followed by classification symbols)

U.S. : 604/96, 97, 104, 132, 133, 891.1; 606/191, 198; 623/1, 11, 12, 13, 900

Documentation searched other than minimum documentation to the extent that such documents are included in the fields searched
NoneElectronic data base consulted during the international search (name of data base and, where practicable, search terms used)
None

C. DOCUMENTS CONSIDERED TO BE RELEVANT

Category*	Citation of document, with indication, where appropriate, of the relevant passages	Relevant to claim No.
X --- Y	WO, A, WO 91/17789 , (STACK ET AL.), 28 November 1991. See entire document.	1-6, 8, 11-13, 15, 16, 19-22 ----- 17, 18

☐ Further documents are listed in the continuation of Box C. ☐ See patent family annex.

* Special categories of cited documents:	*T later document published after the international filing date or priority date and not in conflict with the application but cited to understand the principle or theory underlying the invention
*A document defining the general state of the art which is not considered to be part of particular relevance	*X document of particular relevance; the claimed invention cannot be considered novel or cannot be considered to involve an inventive step when the document is taken alone
*E earlier document published on or after the international filing date	*Y document of particular relevance; the claimed invention cannot be considered to involve an inventive step when the document is combined with one or more other such documents, such combination being obvious to a person skilled in the art
*L document which may throw doubts on priority claim(s) or which is cited to establish the publication date of another citation or other special reason (as specified)	*G document member of the same patent family
*O document referring to an oral disclosure, use, exhibition or other means	
*P document published prior to the international filing date but later than the priority date claimed	

Date of the actual completion of the international search 21 DECEMBER 1993	Date of mailing of the international search report 25 APR 1994
Name and mailing address of the ISA/US Commissioner of Patents and Trademarks Box PCT Washington, D.C. 20231 Facsimile No. NOT APPLICABLE	Authorized officer <i>Vanitha Alexander</i> VANITHA ALEXANDER Telephone No. (703) 308-4987